



TRANSFORMING TECHNOLOGIES

OUTSTANDING ALTERNATIVES IN STATIC CONTROL

How to Test & Evaluate an ESD Worksurface

The Essential Tools and Measurements needed
to Test Your ESD Worksurface

Surface Resistance Meters

Resistance Point-To-Point

Resistance To Groundable Point

Resistance to Ground

Surface Resistance Meters

Surface Resistance Meters send a small current through material and measures the how quickly the current is able to pass through the material and back to the meter. The speed is referred to as the "resistance" of the material i.e. how strongly the material resists charge movement.

Results are measured in Ohms and are typically displayed in powers of 10, also known as decade scale. The lower the number, the more conductive the material.

Materials considered ESD items are in the Dissipative or Conductive range.

Classification	Charge Movement	Resistance	Ohms
Conductive	Very Fast	Low Resistance	10^3 - 10^5
Dissipative	Fast but Slower than Conductive	Medium Resistance	10^6 - 10^{10}
Insulative	Slow or No Movement	High Resistance	10^{11} - 10^{12}

Types:

Resistance meters range from small handled meters, to full kits. All meters include measuring probes that make contact with the material being tested. They are sometimes built-in to the back of the meter or they are external and connected by wires.



Type of Measurements

There are three primary measurements for evaluating a work surface; Resistance Point to Point (RTT – also known as Resistance Top to Top), Resistance to Groundable Point (RTGP) and Resistance to Ground (RTG).

Resistance to Ground Measurement

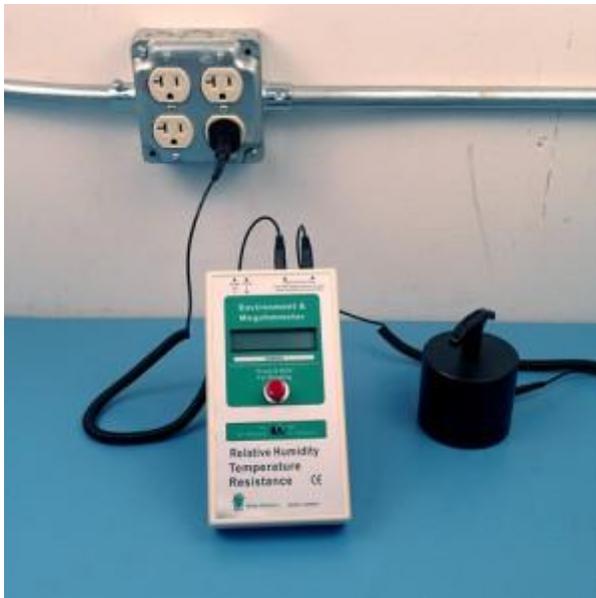


Figure 1 – Resistance To Ground (RTG)

For general auditing purposes, the primary measurement is RTG. This measurement assures that the mat is connected to AC Equipment Ground.

This measurement is made using a 5 lb electrode connected to the positive terminal of the resistance meter. The electrode is placed on the work surface in the most heavily used area. The negative lead is connected to electrical ground.

ESD standard procedure says to test at 10 volts, and if the measurement exceeds 1.0×10^6 ohms, switch to 100 volts. If you are certain that your worksurface material has a resistance greater than 1.0×10^6 ohms, you may want to start at 100 volts to save time.

A simple and safe way to connect to AC Ground is by using a grounding plug, such as the Transforming Technologies AD22. The AD22 assures a solid connection to the third wire ground of an AC outlet, while insulating the plug from the hot and neutral wires. Always check electrical outlets for proper wiring before using grounding plugs.

If the resulting RTG measurement is within your required limits, no further work surface testing is required and you can proceed to the next work surface. Should the RTG measurement exceed your limits, clean the work surface with an approved cleaning product, check all wiring connections to make sure that they are secure and re-test. Should the measurements still exceed your limits you will then want to conduct a Resistance to Groundable Point (RTGP) measurement.

Resistance to Groundable Point Measurement



Figure 2 – Resistance Point To Groundable Point (RTGP)

This measurement is similar to the RTG measurement except that the negative lead is attached to the grounding point (snap) of the work surface. The testing is performed using 100 volts when the expected resistance is greater than 1.0×10^6 ohms.

Should this measurement provide a reading that is within your requirements the problem is somewhere between the snap and AC Ground. Typically, either the ground wire became disconnected or it is faulty. Check and verify all wiring between the work surface and the AC equipment ground.

If this measurement also provides a value that exceeds your requirements, then there may be a problem with the work surface. A point-to-point resistance measurement can be done to verify the performance of the work surface material.

RTT – Resistance Point-to-Point



Figure 3 – Resistance Point To Point (RTT)

This measurement is made using two 5 lb electrodes. The electrodes are placed 10” apart on the work surface in various locations. Figure 3 is an example of a point-to-point test.

The testing is performed using 100 volts when the expected resistance is greater than 1.0×10^6 ohms.

If the reading meets your requirements, there is possibly a connection problem with the groundable point. Should the reading exceed your limits the work surface is likely faulty and should be replaced.

It is important that RTG measurements be made regularly. The frequency of testing is dependent up on internal requirements and testing history. RTG testing must be performed

even if constant monitoring is in place, as constant monitors verify ground connection of the worksurface, but not the performance of the worksurface.

View Transforming Technologies Surface Resistance Meters here:

<http://transforming-technologies.com/product-category/test-equipment/surface-resistance-meters/>

Do you have additional questions? Ask your ESD questions and get answers from certified ESD and Static Control experts:

- **Phone Support: 419-841-9552**
- **Email: info@transforming-technologies.com**
- **Live Chat: <https://purechat.me/cntvd1>**